



## Short title: Minimum safe facilities

### 1. Purpose

This position statement outlines the minimum requirements to be provided by healthcare facilities for safe administration of anaesthesia. It is intended to assist facilities when designing, upgrading, equipping and staffing clinical areas where anaesthesia is delivered. It is recognised that there is an increasingly diverse range of facilities and contexts where anaesthesia is provided, each with its own specific requirements. This document specifies the minimum staffing, equipment, emergency medications and service processes in all locations where anaesthesia is provided.

### 2. Scope

This position statement is intended to apply to operating theatre suites.

It is also intended to apply to any other areas where anaesthesia services may be provided, including standalone facilities and facilities undertaking 'deep sedation', where medications are administered that result in loss of verbal contact with the patient.<sup>1</sup>

It is not intended to apply to intensive care or emergency departments.

Anaesthesia includes general anaesthesia, neuraxial or major regional analgesia as defined in *PG03(A) Guideline for the management of major regional analgesia*, and sedation as defined in *PG09(G) Guideline on sedation and/or analgesia for diagnostic and interventional medical, dental or surgical procedures*.

### 3. Background

Anaesthesia spans the perioperative period, and it is essential that all aspects of management involved in each phase relevant to the healthcare facility can be safely provided. It is expected that healthcare facilities providing anaesthesia services meet the minimum requirements contained within this Position Statement and engage the services of qualified medical practitioners' credentialed in accordance with ANZCA *PS02(A) Position statement on credentialling and defining the scope of clinical practice in anaesthesia*.

### 4. Staffing

Whenever anaesthesia is being administered there should be a dedicated assistant for the anaesthetist in accordance with ANZCA professional document *PS08(A) Position statement on the assistant for the anaesthetist*.

There should be sufficient assistance immediately available for the duration of the procedure for positioning the patient in accordance with the occupational health and safety regulations of the facility. As a minimum this should be three, although more may be required depending on the physical characteristics of the patient, staff, and patient transfer device.

Trained and qualified technical assistants to ensure proper functioning and servicing of all relevant equipment should be available.

---

<sup>1</sup> Refer to Document Framework Policy Glossary section for a full description of deep sedation.

## 5. Physical location

### 5.1 Pre-anaesthesia consultation.

ANZCA *PG07(A) Guideline on pre-anaesthesia consultation and patient preparation* outlines the facilities required to fulfil this task.

### 5.2 Post-anaesthesia care unit – post-anaesthesia recovery.

ANZCA *PS04(A) Position statement on the post-anaesthesia care unit* outlines the design, equipment, and staffing required to deliver safe patient care.

### 5.3 Anaesthetising locations.

It is a requirement that all facilities comply with regulatory and licensing standards as well as occupational health and safety regulations including:

- Lighting and emergency lighting
- Electric power supply with backup
- Patient transfer devices to assist with safe transfer of patients from the procedural table to the recovery trolley, and then safe transport to the recovery area (refer ANZCA *PS04(A) Position statement on the post-anaesthesia care unit*).

Other requirements include:

- Availability of telecommunications permitting communication with persons outside the anaesthetising location. Ideally, there should also be mobile phone reception and internet access
- Presence of an anaesthesia emergency call system
- Heating/cooling sufficient to maintain theatre temperature at a specified temperature within the range 18-28°C
- Equipment to ensure safe positioning of patients during procedures
- Secure but accessible storage for restricted medications according to jurisdictional requirements

### 5.4 Evacuation

Contingency plans should exist for the safe and timely emergency evacuation of patients from the operating suite and/or recovery areas under medical supervision.

## 6. Equipment

### 6.1 Essential anaesthesia equipment

Monitoring of physiological and other variables should comply with ANZCA professional document *PG18(A) Guideline on monitoring during anaesthesia*. The availability of equipment for invasive monitoring will be determined by patient complexity in addition to surgical or procedural complexity and may even be required for straightforward procedures.

The equipment listed below is regarded as essential, however, the specific requirements should be tailored to the types of procedures and patients in the facility.

Each facility should designate at least one credentialed specialist anaesthetist to advise on the choice and maintenance of anaesthesia equipment and at least one of its nursing or technical staff to be responsible for organising, maintaining, and servicing anaesthesia equipment.

Personal protective equipment and theatre clothing appropriate for both the designated procedure and for the patient population undergoing care, must be provided for all personnel. This includes protection from biological hazards such as contaminated body fluids, equipment to

reduce the risk of healthcare related infections<sup>2</sup> (see *PG28(A) Guideline on infection control in anaesthesia*) as well as equipment to reduce exposure to physical hazards such as laser eye protection and ear protection where needed.

It is highly recommended that laminated copies of cognitive aids and flowcharts be available and accessible in each location. These should include management of can't intubate can't oxygenate (CICO), anaphylaxis, cardiac arrest, systemic local anaesthetic toxicity and malignant hyperthermia emergencies.

Basic airway equipment related to the types of patients and procedures include:

- Facemasks
- Airway adjuncts (oropharyngeal and nasopharyngeal airways)
- At least two laryngoscopes
- A range of tracheal tubes
- Supraglottic airways
- Connectors, bougies/introducers and associated equipment suitable for the size and age of patients to be anaesthetised
- Magill's forceps
- Throat packs,
- Syringes for inflation of tracheal tube and supraglottic airway cuffs and sterile lubricant for airway devices
- High flow airway equipment to provide support during shared airway and deep sedation procedures

As a minimum, the following should also be available:

- Additional advanced airway equipment should also be provided in a separate difficult airway trolley as outlined in *PG56(A) Guideline on equipment to manage difficult airways* including a pre-prepared kit for performance of an emergency front of neck airway procedure in case of a can't intubate, can't oxygenate crisis.
- A separate means of inflating the lungs with oxygen that complies with the current relevant national standard and is independent of the anaesthesia delivery system. The size of any device and its attachments will be determined by patients being anaesthetised at any given location.
- Suction apparatus that complies with the current relevant standard for the exclusive use of the anaesthetist at all times together with hand pieces and endotracheal suction catheters. There should be provision for an alternative suction system in the event of primary suction failure.
- Equipment for intravenous cannulation (tourniquets, skin preparation and cannulae) including means for safe disposal of sharps and minimisation of infection as outlined in *PG28(A) Guideline on infection control in anaesthesia*. Adhesive tapes and scissors should be provided to secure intravascular and airway devices.
- A stethoscope and manual sphygmomanometer
- Monitoring equipment as identified in ANZCA professional document *PG18(A) Guideline on monitoring during anaesthesia*.
- A cardiac defibrillator with capacity for synchronised cardioversion. In larger centres or centres with patients with complex co-morbidities there should be provision for transcutaneous pacing.
- Equipment for sub-arachnoid, epidural or regional nerve blocks, where required.

## 6.2 Context-specific anaesthesia equipment

In addition to these basic requirements, additional provisions should be made for areas where specific types of surgery or anaesthesia are performed.

6.2.1 Where volatile anaesthesia is delivered, or non-depolarising muscle relaxants used the following are essential:

---

<sup>2</sup> Refer to [ANZCA statement on personal protection equipment \(PPE\)](#)

- An anaesthesia delivery system or anaesthesia machine with a gas scavenging system that complies with *PS54(A) Position statement on the minimum safety requirements for anaesthesia machines and workstations for clinical practice*.
- Breathing systems including paediatric breathing systems if paediatric patients are to be anaesthetised.
- Equipment for automatic ventilation of the lungs, incorporating alarms as specified in ANZCA professional document *PG18(A) Guideline on monitoring during anaesthesia*.

6.2.2 Where anaesthesia is delivered by intravenous infusion the following are strongly recommended:

- Equipment for programmable delivery of medication by infusion, preferably loaded with applicable pharmacokinetic models.
- Depth of anaesthesia monitoring such as a processed electroencephalogram monitor if muscle relaxation is also employed.

6.2.3 Where complex surgery is undertaken such as cardiac, thoracic, major vascular neurosurgery or obstetrics the following are essential:

- Equipment for the direct measurement of arterial and venous pressures.
- Equipment for the rapid infusion of fluids such as manual pump giving sets and devices to heat and pressurise fluid.
- Interpleural drainage sets including underwater seal drainage equipment or one way valves in facilities where thoracic trauma or surgery is undertaken, or where there may be a risk of pneumothorax.
- Equipment for the active warming (and where appropriate, cooling) of patients such as insulating sheets, forced air warming devices, mattress warmers and intravenous fluid warmers.

6.2.4 Where oxygen is administered to patients undergoing sedation in the presence of diathermy refer to Appendix 3.

## 7. Emergency medications

In addition to the medications and agents commonly used to manage anaesthesia, medications should also be available for the management of emergencies arising as a result of, or in associations with, anaesthesia. For a list of these conditions and the recommended list of medications refer to Appendix 1.

In addition, if volatile anaesthetics or suxamethonium are intended to be used, the possibility of malignant hyperthermia (MH) is present. A supply of Dantrolene appropriate to the clinical area must be stocked. Recommended levels for stock are outlined in Appendix 2. MHAZ and AAGBI recommend dantrolene administration continue until end-tidal carbon dioxide is < 45 mmHg and core temperature is <38.5°C. In this setting capnography and core temperature monitoring availability is critical<sup>3</sup>.

## 8. Related ANZCA documents

PS02(A) Position statement on credentialling and defining the scope of clinical practice in anaesthesia

PS04(A) Position statement on the post-anaesthesia care unit

PG07(A) Guideline on pre-anaesthesia consultation and patient preparation

PS08(A) Position statement on the assistant for the anaesthetist

---

<sup>3</sup> AAGBI guidelines Malignant hyperthermia 2020.

<https://anaesthetists.org/Portals/0/PDFs/Guidelines%20PDFs/Guideline%20Malignant%20hyperthermia%202020.pdf?ver=2021-01-13-144236-793>

PG18(A) Guideline on monitoring during anaesthesia

PG28(A) Guideline on infection control in anaesthesia

PG31(A) Guideline on checking anaesthesia delivery systems

PS54(A) Position statement on the minimum safety requirements for anaesthesia machines and workstations for clinical practice

PG56(A) Guideline on equipment to manage difficult airways

**This document is accompanied by a background paper (PS55(A)BP) which provides more detailed information regarding the rationale and interpretation of the position statement.**

*Professional documents of the Australian and New Zealand College of Anaesthetists (ANZCA) are intended to apply wherever anaesthesia is administered and perioperative medicine practised within Australia and New Zealand. It is the responsibility of each practitioner to have express regard to the particular circumstances of each case, and the application of these ANZCA documents in each case. It is recognised that there may be exceptional situations (for example, some emergencies) in which the interests of patients override the requirement for compliance with some or all of these ANZCA documents. Each document is prepared in the context of the entire body of the College's professional documents, and should be interpreted in this way.*

*ANZCA professional documents are reviewed from time to time, and it is the responsibility of each practitioner to ensure that he or she has obtained the current version which is available from the College website ([www.anzca.edu.au](http://www.anzca.edu.au)). The professional documents have been prepared having regard to the information available at the time of their preparation, and practitioners should therefore take into account any information that may have been published or has become available subsequently.*

*Whilst ANZCA endeavours to ensure that its professional documents are as current as possible at the time of their preparation, it takes no responsibility for matters arising from changed circumstances or information or material which may have become available subsequently.*

Promulgated (as T1):	1978
Reviewed:	1984, 1989, 1994, 1995, 2000, 2006, 2008
Republished:	2012 (rebadged from T01 to PS55)
Current document:	Aug 2021
Appendix 1 & 2	2021
Appendix 3	2024

© Copyright 2021 – Australian and New Zealand College of Anaesthetists. All rights reserved.

*This work is copyright. Apart from any use as permitted under the Copyright Act 1968, no part may be reproduced by any process without prior written permission from ANZCA. Requests and inquiries concerning reproduction and rights should be addressed to the Chief Executive Officer, Australian and New Zealand College of Anaesthetists, 630 St Kilda Road, Melbourne, Victoria 3004, Australia. Email: [ceoanzca@anzca.edu.au](mailto:ceoanzca@anzca.edu.au)*

Website: [www.anzca.edu.au](http://www.anzca.edu.au)



## Appendix 1 - Emergency medications

Some of the emergency conditions that may be encountered and therefore preparations should be made include adrenal dysfunction, anaphylaxis, bronchospasm, cardiac arrest, cardiac arrhythmias, coagulopathies, hyperkalaemia, hypoglycaemia, hypotension, hyperglycaemia, hypertension, malignant hyperpyrexia, major Haemorrhage, pulmonary oedema, raised intracranial pressure, respiratory depression, and uterine atony (where relevant).

A **minimum** requirement for basic emergency medication inventories “should include”:

- Adrenaline/Epinephrine (1mg in 1ml) x3
- Adrenaline/Epinephrine (1mg in 10ml) x3
- Amiodarone (total of 450mg)
- Atropine (total of 3mg)
- Dantrolene (as per recommendation below)
- Dextrose 50%
- Ephedrine (30mg) x3
- Ergometrine (obstetrics)
- Esmolol
- Furosemide (total of 100mg)
- Glucagon (1mg/1iu)
- Glyceryl Trinitrate (total 50mg)
- Hydrocortisone (100mg) x2
- Insulin (short acting)
- Intralipid
- Magnesium (10mmol in 5 ml) x 2
- Metaraminol (10mg) x3
- Metoprolol IV (5mg) x2
- Naloxone (400mcg)
- Noradrenaline/Norepinephrine (total 3mg)
- Oxytocin (10iu) x5 (as required)
- Phenylephrine (as required)
- Prostaglandin F2a (as required)
- Salbutamol Metered Dose Inhaler
- Salbutamol iv
- Suxamethonium (100mg) x2
- Tranexamic Acid (1g) x2





## **Appendix 2 - Malignant hyperthermia**

It is an MHA NZ recommendation that Dantrolene be stocked in any anaesthetising location using volatile anaesthesia, or where suxamethonium is planned to be used (other than for airway emergencies).

It is also recommended that an initial dose of at least 180mg of dantrolene be available to all locations within 5 minutes of an emergency. Subsequent doses of dantrolene should be available so that an additional 180mg is available every 15 minutes thereafter up to a total of 720mg doses. In other words, 180mg of dantrolene must be available within 5 minutes, 360mg available within 20 minutes, 540mg available within 35 minutes, and 720mg available within 50 minutes.

These doses are to be reliably available within the specified timeframes to any location at any time when anaesthesia is being delivered. Facilities should have a specific and accessible plan for obtaining further dantrolene if more than 720mg is required.



## Appendix 3 - Non-airway burns/fires in the operating room

### Purpose

To guide anaesthetists, operating room staff and surgeons in preventing and managing non-airway non-intrathoracic fires in the operating room.

### Scope

This appendix applies to preventing and managing patient-related non-airway burns/fires associated with the use of supplemental oxygen in the operating room.

### Definitions

Non-airway burns/fires occur outside the airway and do not involve airway surgery.

### Background

Fires in the operating room are relatively rare; however, they pose a significant threat to patient and staff safety and can result in severe injuries or even fatalities. In addition, fires might spread beyond the immediate area and require the evacuation of the operating room or even the hospital [1]. In the American Society of Anesthesiologists (ASA) Closed Claims Database, up until 2013, 103 OR fires accounted for 1.9% of the total surgical claims and typically occurred in older patients [2]. It is estimated that there are 88-650 cases per year [3,4] in the United States, with an incidence of 0.2-0.8 surgical fires per 100,000 surgical procedures [5].

The local webAIRS reporting system [6] showed the most frequent thermal injuries were observed in the head and neck areas during superficial surgical procedures performed under monitored anaesthesia care, specifically in the fields of plastic surgery, vascular surgery, and cardiology. These injuries represented 50% of the total thermal injuries reported. Ten cases were linked to using an open system to deliver supplemental oxygen, harming the patient's face and airway. This harm included six superficial burns, accounting for 60% of the injuries, two partial-thickness burns, making up 20%, and two inhalational injuries, also at 20%. Various oxygen delivery devices were involved in these incidents, such as simple face masks (50%), low-flow nasal prongs (10%), and high-flow nasal prong devices with humidification (40%). The concentration of oxygen provided by these devices varied, with FiO<sub>2</sub> levels ranging from approximately 30% to 100% and flow rates from 3L/min to as high as 70L/min.

These fires typically involve the ignition of flammable substances, such as surgical drapes, alcohol-based skin preparations, or even the patient's body tissues in an oxygen-enriched atmosphere.

The fire triangle or triad [7,8] is a concept used to illustrate the three elements that are necessary for a fire to occur: fuel, an oxidiser (typically oxygen), and an ignition source.

1. **Fuel:** Fuel refers to any material that can burn. It can be a solid, liquid, or gas. Common examples of fuel in the operating room include surgical drapes, alcohol-based skin preparations, flammable gases such as methane (e.g. in the patient's bowel), and other flammable substances such as clothing or hair [9].
2. **Oxidiser:** This supports the chemical reactions that occur during a fire, with oxygen being the most common oxidiser, followed by nitrous oxide. In the medical setting, supplemental oxygen is used, leading to oxidised-enriched atmospheres, which can significantly increase the risk and hasten [10-12] the intensity of fires, especially as concentrations increase [10,13,14]. Fires may occur with an open delivery system during monitored anaesthetic care in the head, neck and upper chest surgical fields [2,15].
3. **Ignition Source:** An ignition source is any heat source capable of raising the temperature of the fuel to its ignition point. The most common ignition source is the monopolar diathermy attached to an



electrosurgery unit. Still, it can also include any heat-generating device such as a bipolar diathermy [2], lasers, fibre optic light sources, drills or, occasionally, a cardiac defibrillator.

**Prevalence and risk factors:**

Certain procedures carry a higher risk of fires, such as those involving head, neck, or upper chest surgeries [2,5]. These include plastic surgery on the face (64%), miscellaneous neck procedures (12%), temporal artery biopsy (8%), upper chest procedures such as a pacemaker or central line insertion (6%), and carotid endarterectomy under local and sedation (3%) [2].

Factors that increase the likelihood of fire include the presence of an open oxygen source with a higher proportion in nasal cannula oxygen administration [2], which produced greater than expected oxygen concentration, especially at higher flow rates [16-18] or dislodgement of the cannula [19], the concentration of the oxidiser in the immediate area [11] especially if greater than a FiO<sub>2</sub> of 0.3 [20], the use of flammable materials or facial hair or eyebrows [9], the proximity of the ignition source to the fuel, and inadequate communication by the operating room team [2].

It should be noted in a small ophthalmic plastic study sampling oxygen concentration around the eyes that a correctly fitted nasal cannula resulted in no oxygen-rich environment compared with an oxygen-rich environment (24.3 - 33.8% average oxygen concentrations) when facemasks were used. However, no flow rate is mentioned [21]. Furthermore, another study showed that at a flow of 2 l/min, oxygen concentrations exceeded 23% only within a few centimetres of the nasal cannula and that concentration increased as a flow function [17]. It was recommended that all ignition sources should be kept at least 10 cm away from the oxygen source when using flow rates greater than 4 l/min with a nasal cannula or restricting the oxygen flow to less than 3 l/min. However, a surgical fire occurred when a patient received oxygen administered via a single nasal sponge cannula at low flow (2 l/min), albeit after monopolar diathermy was applied [22].

**Christiana Fire Risk Assessment Score System [23]**

This is a rapidly performed simple 3-point scoring system developed to identify operations at increased risk of surgical fires and to heighten awareness around prevention, which should ideally be performed during the time-out process.

Surgery above the xiphoid:	1 point
Open oxygen source:	1 point
Available ignition source	1 point

Total Points

Low risk for a surgical fire	1 point
Medium risk for a surgical fire	2 points
High risk for a surgical fire	3 points

**Prevention**

Preventing fires in the operating room involves implementing robust safety protocols. These measures include conducting thorough fire risk assessments, ensuring proper communication and coordination among the surgical team, maintaining a clutter-free environment, and using non-flammable surgical drapes and equipment whenever possible. Additionally, carefully administering supplemental oxygen and properly handling flammable substances are crucial in reducing the risk of fires.

1. Shared decision-making and communication:
  - Effective communication and shared decision-making between anaesthetists, surgeons, and nursing staff are crucial to minimise the risk of surgical fires.
  - The risk factors for fires, including oxygen concentration, ignition sources, and available fuel, should be addressed in pre-operative discussions.
  - This conversation should emphasise the importance of safety and the optimisation or discontinuation of supplementary oxygen delivery throughout the various stages of the surgical procedure.
  
2. Institutional considerations.

- Communication regarding fire risk levels should be discussed at the beginning of the list or time-out process, and a strategy should be implemented to prevent or reduce the risk of it happening: refer to [Communicating for Safety Standard](#).
- Designated Staff should be trained in the selection and use of fire extinguishers.
- Fire and Evacuation policies
- Equipment availability
- Structural safety to minimise risks:
  - i. Fire extinguisher availability and location
  - ii. Fire blanket availability and location
  - iii. Automatic Sprinkler and misting systems
  - iv. Low-level lighting
  - v. Access to fire safety equipment
  - vi. Fire Smoke and Audio alarms
  - vii. Signage
  - viii. ISO Australian Health Safety Guidelines
  - ix. Certification of fire safety
  - x. Ensuring evacuation routes are kept clear.
  - xi. Communication with Fire Services
  - xii. Operating theatres are designed so that most operating theatres remain unaffected by fire should one occur, and they should be separated by a 30-minute fire-rated sub-compartment [1].
  - xiii. Evacuation boxes

The National Construction Code Volume One Building Code of Australia 2022 defines hospitals as Class 9a buildings where occupants require assistance to be evacuated. The performance-based design brief is prepared by consultation between a fire safety engineer, architect, fire service, appropriate authority, client, and tenants. It is the plan that specifies what is required. The appropriate number and locations for fire hose reels and hydrants to cover the whole building, as well as fire extinguishers that cover Class A (flammable materials) and E (Electrical) fires, should be available. Typical in the operating area, this is a CO<sub>2</sub> one, which should be tested every six months and recharged every five years.

### 3. Anaesthetic considerations.

- Supplemental oxygen should only be administered when indicated and at the lowest necessary dose to maintain patient oxygenation after the local anaesthesia has been infiltrated.
- If supplemental oxygen is required, consideration should be given to intermittent oxygen administration when diathermy is not in use, and the diathermy time should possibly be limited if the patient's oxygenation is not maintained with this method. However, it might be better to use a closed system administration if oxygenation is not maintained.
- If concerned about fire risk, use a closed system with a cuffed endotracheal tube or a partially closed system with a supraglottic airway. Consider securing the airway with a supraglottic airway or with tracheal intubation if there are concerns about fire risk and for procedures above the xiphoid or if >30% oxygen is used.
- Ongoing high-flow nasal oxygen (HFNO) is not recommended during local and sedation procedures in the head and neck region involving an ignition source (diathermy), and the minimum amount of oxygen supplementation required to keep the patient's oxygen saturation at a reasonable level is the aim [24]. If necessary, an oxygen air blender can be used if the oxygen concentration required is less than 30%. If a higher concentration is required, consider securing the airway.
  - i. Specifically, Fisher and Paykel Healthcare provide the following advice regarding their high-flow nasal oxygen system to avoid fire and burns: From their FIRE DANGER information [25].
    - This product is an open oxygen delivery system.
    - Open oxygen delivery can increase the risk of a surgical fire occurring, causing serious injury or death. Extreme care must be taken.
    - **Contraindication:** Do not use this product with electrosurgery or electrocautery devices on the head or neck.
    - **Warning:** Do not use this product where ignition sources and fuel are present.

- One small study of 10 people showed that the ambient airway rapidly dilutes HFNO-administered oxygen and does not cause an increased oxygen-enriched environment around the chest [26]. However, this should be interpreted cautiously, as a chest fire in the setting of HFNO has been reported (personal communication).

#### 4. Surgical considerations.

- Ideally, do not use an ignition source (diathermy) near supplementary oxygen.
- Single operator diathermy use [27].
- Utilising the lowest effective power [27].
- minimising time in cutting mode (cutting mode generates higher temperatures than coagulation mode) [27],
- using bipolar diathermy rather than monopolar (whilst this does not obliterate the risk of ignition entirely, there is less current leakage with bipolar; therefore, it is preferable) [27]
- Keep diathermy in a sheath when not in use.
- To prevent oxygen pooling, it is important to ensure properly configured surgical drapes and avoid leaving any space where oxygen can accumulate, as oxygen, being heavier than air, tends to pool beneath the drapes. [11,27,28].
- Consider draping the surgical field with wet, saline-soaked packs or ensure that wet packs and saline are available to help extinguish a fire.
- If surgery is close to the oxygen source, consider 'open' draping or placing a plastic barrier apron on patients to prevent oxygen enrichment in clothing and bedding [29]. However, occlusive drapes (e.g. for ophthalmic surgery) may be falsely reassuring as they may still have gaps that allow oxygen to travel to the proximity of the surgical site [30].
- Consider using a scavenger system to prevent excessive pooling of oxygen near the surgical site [31].
- Minimise burn eschar [28].
- Fire retardant surgical drapes [32]
- Consider avoiding alcohol preparations [32-35] for superficial procedures by using an antiseptic solution such as povidone-iodine solution or aqueous chlorhexidine instead. If an alcohol preparation is indicated, use minimal amounts, avoid pooling of the alcohol preparation, and allow at least 3 minutes of time to dry so the alcohol can evaporate [28]. However, this doesn't guarantee that a fire will not happen [35], and longer may be required in people with a lot of hair. There should be an assessment before starting the operation for the pooling of the prep solution [35].

### **Management of a non-airway fire/burn**

Despite preventative measures, fires can still occur in the operating room. Immediate and effective response is critical to minimising harm. The operating team should be trained in fire response protocols, including stopping the procedure, removing the ignition source, and extinguishing the fire with fire extinguishing agents designated for the purpose, providing it is safe. Patient and Staff safety and evacuation take precedence over extinguishing the fire if it is not small, controllable, and self-contained. Be aware that flame from ongoing combustion (especially alcohol) may be hard to see in a brightly lit operating theatre.

#### 1. Immediate [36]

- Stop diathermy.
- Stop additional oxygen supplementation to reduce FiO<sub>2</sub> to 0.21
- Call for help.
- Remove drapes and burning material.
- Flood the fire with saline or saline-soaked gauze and then institute a cutaneous burn treatment with cold running water for at least 20 minutes within the first 3 hours [37]. If this is unrealistic (eg on the face), then regularly changed wet packs should be applied.
- Use a carbon dioxide fire extinguisher.
- Consider closing the oxygen shut-off valves and evacuation plans if the fire is ongoing.

Alternatively, use:

### **RACE Principles**

- R     Remove/Rescue  
Remove drapes and burning material or rescue any people in immediate danger only if it is safe to do so.
- A     Alarm/Alert  
Raise the alarm, notify your switchboard and the staff member in charge or fire warden to escalate referral to fire service as required.
- C     Contain  
If practicable, close all doors and windows to contain the fire.
- E     Extinguish/Evacuate  
Try to extinguish the fire using firefighting equipment, but only if you are trained and it is safe to do so. Otherwise, evacuate if uncontrolled.
2. Ongoing patient management
- Stabilisation – Re-establish ventilation, minimising oxygen and avoiding nitrous oxide. Assess the damage and consider inhalational injuries and whether intubation is required for ongoing management [36].
  - Referral
  - Transfer
  - Open Disclosure
3. Review
- Fire compartments/oxygen shut-off valves for the specific areas.
  - Evacuation plans (should include laminated action cards suitable for the local environment)

### **Open disclosure**

Open disclosure in the healthcare context involves how clinicians communicate with and support patients, their families, and caregivers who have experienced harm during their healthcare journey.

In Australia, the Australian Charter of Healthcare Rights and in New Zealand, Health & Disability Commissioner Te Toihau Hauora, Hauatanga, outlines patients' specific rights during the open disclosure process.

These rights empower patients to actively participate in their healthcare, ensure transparency and accountability within the healthcare system, and promote a culture of continuous improvement in patient safety and quality of care.

### **Awareness and education**

Continuous education and awareness programs ensure that healthcare professionals remain vigilant about fire risks in the operating room. These programs should emphasise the potential hazards, preventive measures, proper response protocols, and the importance of teamwork during fire emergencies.

Practical in-house training programs [38], including the locations of fire extinguishers, oxygen shut-off valves, fire call points and evacuation plans, should be included in the orientation and ongoing education of staff, ideally in a multi-disciplinary setting [1]. This should occur on an annual basis for regular full-time staff.

### **Summary of Key Points for Fire Safety in Sedation and Surgery around the Face, Head, or Neck [7,39]**

1. **Plan:** The anaesthetist and surgeon need to consider and discuss the level of sedation and the patient's oxygen requirements for the proposed procedure.

2. **Brief:** Appraise and discuss the plan and potential for risks (including using a risk assessment tool eg Christiana (above)) with the whole team. This includes confirming that all understand the institution's fire management protocol before commencing the operating list.
3. **Select** the appropriate oxygen delivery system (see also attached algorithm):
  - a. For moderate or deep sedation or oxygen-dependent patients, consider using a closed or partial closed system (cuffed tracheal tube or supraglottic airway)
  - b. For light sedation, an open system such as a facemask or nasal cannula may be suitable, though HFNO should be used with great caution, and a closed system may be a better option than HFNO.
    - i. It should be noted that the oxygen concentration increases as the flow rate increases. Therefore, the flow rates should ideally be below 3 l/min, and if using more than 4 l/min, the operation should be greater than 10 cm away [17], or a closed system should be considered.
    - ii. There is conflicting evidence about whether a facemask or nasal cannula is a safer option. More airway fires in the US occurred with a nasal cannula [2]. However, in oculoplastic practice, a correctly fitted nasal cannula resulted in lower oxygen concentrations than the facemask around the eyes [21], and a flow rate was not mentioned.
4. **Alert:** The surgeon should inform the anaesthetist in advance before activating any ignition sources near the face, head, neck or chest.
5. **Assess:** The oxygen delivery should be evaluated if it is still required after any local anaesthetic administration and stopped. If oxygen is still required, it should be reduced to the minimum required to prevent hypoxia.
6. **Confirm:** The operating room team should check that the oxygen supplementation has been minimised or stopped.
7. **Wait:** Allow time for oxygen concentration to be reduced (dissipate) before commencing the surgery.

### **Cognitive aid algorithm**

A cognitive aid is provided in the form of a flow chart identifying the key steps and decision points to aid decision making regarding oxygen delivery.


### **Explicit recommendation:**

If the patient requires ongoing oxygen supplementation in the setting of a high-fire risk ie 3 points (with or without sedation), consideration should be given to converting to a general anaesthetic and securing the patient's airway with a well-sealed supraglottic airway or endotracheal tube.



**ANZCA**  
FPM

# Fire Prevention Algorithm

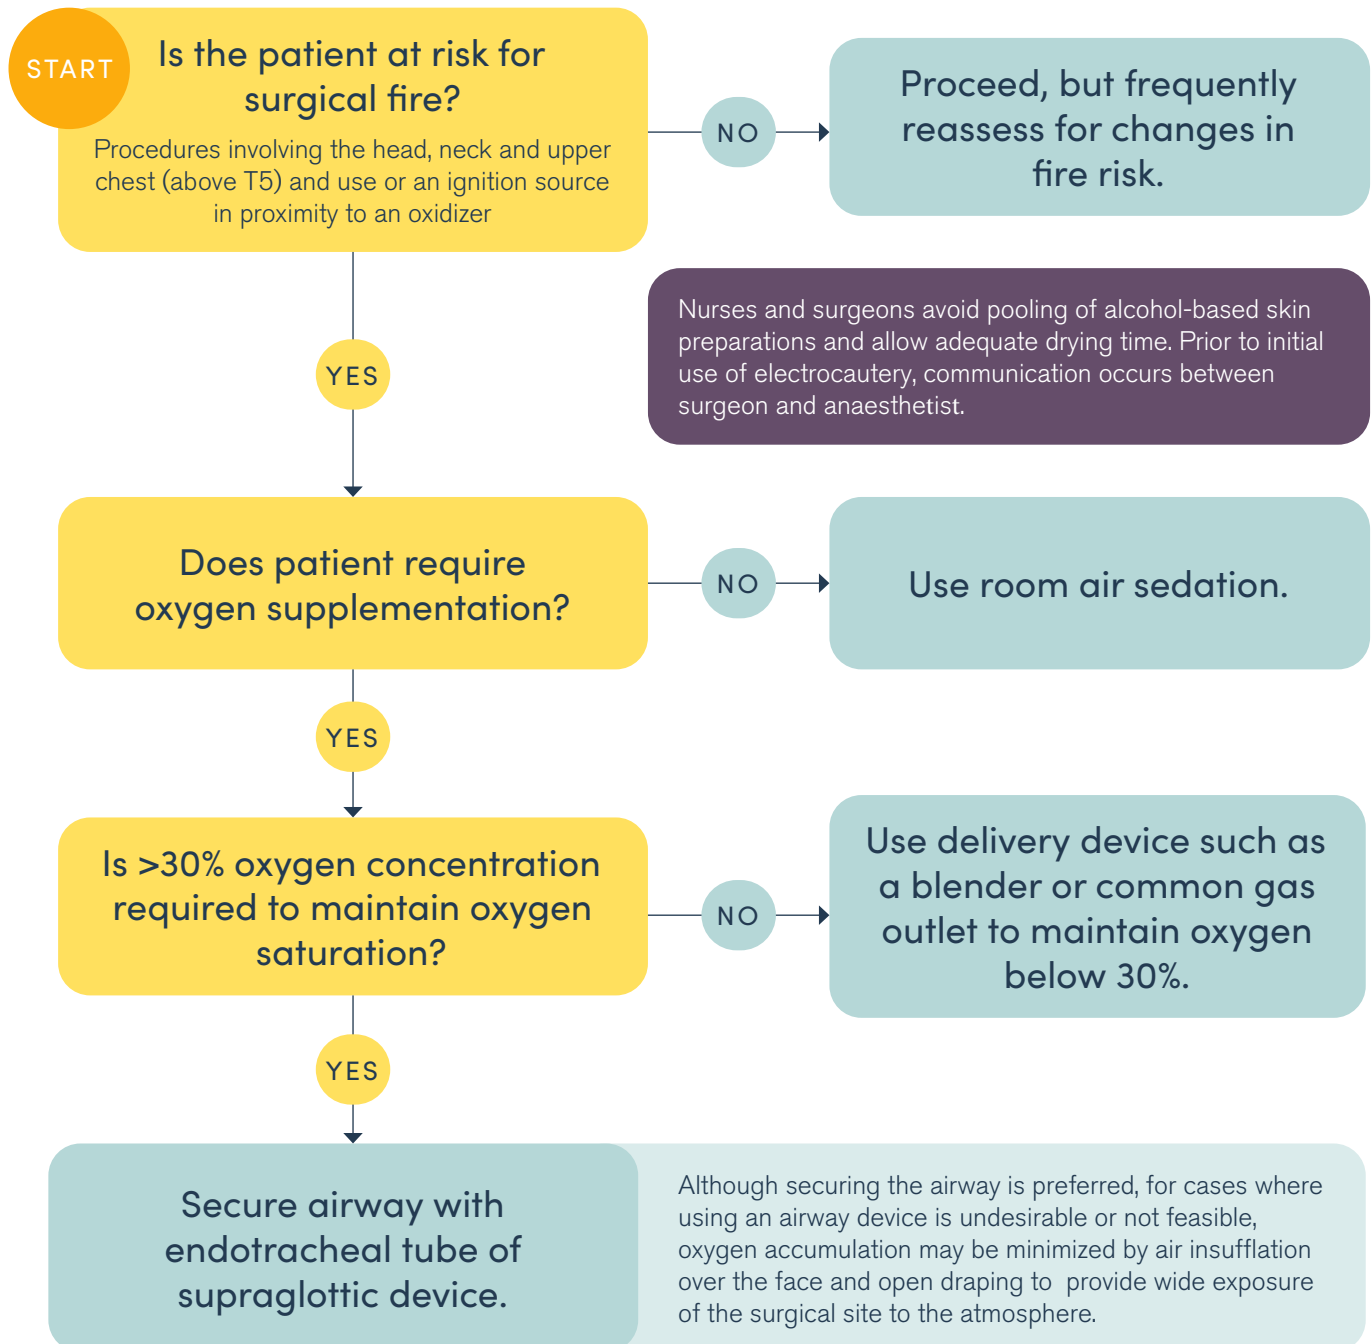



## References

1. Kelly FE, Bailey CR, Aldridge P, et al. Fire safety and emergency evacuation guidelines for intensive care units and operating theatres: for use in the event of fire, flood, power cut, oxygen supply failure, noxious gas, structural collapse or other critical incidents: Guidelines from the Association of Anaesthetists and the Intensive Care Society. *Anaesthesia* 2021; **76**: 1377-91.
2. Mehta SP, Bhananker SM, Posner KL, Domino KB. Operating room fires: a closed claims analysis. *Anesthesiology* 2013; **118**: 1133-9.
3. Institute E. New clinical guide to surgical fire prevention. Patients can catch fire--here's how to keep them safer. *Health Devices* 2009; **38**: 314-32.
4. Group SLW. A case for the prevention and management of surgical fires in the UK. Expert Working Group Recommendations, 2020. [https://www.afpp.org.uk/news/A\\_case\\_for\\_the\\_prevention\\_and\\_management\\_of\\_surgical\\_fires](https://www.afpp.org.uk/news/A_case_for_the_prevention_and_management_of_surgical_fires) (accessed 12/07/2023).
5. Bruley MA, T; Finley, E; Deutsch, E; Treadwell, J. Surgical Fires: Decreasing Incidence Relies on continued Prevention Efforts: PA Patient Saf Advis., 2018: 1-12.
6. Steer A. Burns in the operating theatre! a webinars review *Australian Anaesthetist*. Australian Society of Anaesthetists, 2023: 44 -6.
7. Apfelbaum JL, Caplan RA, Barker SJ, et al. Practice advisory for the prevention and management of operating room fires: an updated report by the American Society of Anesthesiologists Task Force on Operating Room Fires. *Anesthesiology* 2013; **118**: 271-90.
8. Kezze I, Zoremba N, Rossaint R, Rieg A, Coburn M, Schalte G. Risks and prevention of surgical fires : A systematic review. *Anaesthetist* 2018; **67**: 426-47.
9. Schulz EB, Bright MR. Fire risk when using high-flow nasal oxygen during procedural sedation. *Anaesthesia* 2023; **78**: 396.
10. Goldberg J. Brief laboratory report: surgical drape flammability. *Aana j* 2006; **74**: 352-4.
11. Greco RJ, Gonzalez R, Johnson P, Scolieri M, Rekhopf PG, Heckler F. Potential dangers of oxygen supplementation during facial surgery. *Plast Reconstr Surg* 1995; **95**: 978-84.
12. Howard BK, Leach JL. Prevention of flash fires during facial surgery performed under local anesthesia. *Ann Otol Rhinol Laryngol* 1997; **106**: 248-51.
13. Wolf GL, Sidebotham GW, Lazard JL, Charchaflieh JG. Laser ignition of surgical drape materials in air, 50% oxygen, and 95% oxygen. *Anesthesiology* 2004; **100**: 1167-71.
14. Culp WC, Jr., Kimbrough BA, Luna S. Flammability of surgical drapes and materials in varying concentrations of oxygen. *Anesthesiology* 2013; **119**: 770-6.
15. Barker SJ, Polson JS. Fire in the operating room: a case report and laboratory study. *Anesth Analg* 2001; **93**: 960-5.
16. Barnes AM, Frantz RA. Do oxygen-enriched atmospheres exist beneath surgical drapes and contribute to fire hazard potential in the operating room? *Aana j* 2000; **68**: 153-61.
17. Orhan-Sungur M, Komatsu R, Sherman A, Jones L, Walsh D, Sessler DI. Effect of nasal cannula oxygen administration on oxygen concentration at facial and adjacent landmarks. *Anaesthesia* 2009; **64**: 521-6.
18. Engel SJ, Patel NK, Morrison CM, et al. Operating room fires: part II. optimizing safety. *Plast Reconstr Surg* 2012; **130**: 681-9.
19. Reyes RJ, Smith AA, Mascaro JR, Windle BH. Supplemental oxygen: ensuring its safe delivery during facial surgery. *Plast Reconstr Surg* 1995; **95**: 924-8.
20. APSF. Operating Room Fire Safety Video, 2010. <https://www.apsf.org/videos/or-fire-safety-video/> (accessed 11/07/2023).
21. Huddleston S, Hamadani S, Phillips ME, Fleming JC. Fire risk during ophthalmic plastic surgery. *Ophthalmology* 2013; **120**: 1309 e1.
22. Saha K, Ataullah S, Slater R. Fire risk during eye surgery. *Anaesthesia* 2010; **65**: 1046-7.
23. CCHS. Surgical fire risk assessment. <https://christianacare.org/us/en/for-health-professionals/education/surgical-fire-risk-assessment> (accessed 11/07/2023).
24. Cooper JG, B; Ehrenwerth, J. Safe Use of High-Flow Nasal Oxygen (HFNO) With Special Reference to Difficult Airway Management and Fire Risk. *APSF Newsletter* 2018; **October**: 51-3.
25. Instructions. OptiflowTM+ Nasal Cannula User Instruction: Fisher & Paykel Healthcare Limited, 2021.
26. Seki H, Fukagata K, Ito S, Okada R, Ouchi T. Effect of high-flow nasal oxygen use on oxygen flow at the surgical site: a pilot study. *Br J Anaesth* 2021; **127**: e192-e5.
27. Ward P. THRIVE and airway fires. *Anaesthesia* 2017; **72**: 1035.
28. Greenland KB. High Flow Nasal Oxygen and Fire Risk - Cautionary note on device usage. *ANZCA Bulletin* 2018; **March 2018**: 25-6.

29. Jones TS, Black IH, Robinson TN, Jones EL. Operating Room Fires. *Anesthesiology* 2019; **130**: 492-501.
30. Feldman JC, C. Experts Respond: Occlusive Drapes Unreliable as O2 Barrier: Insufflate With Air or <30% FiO2 for Patient Comfort. *APSF Newsletter* 2012; **Fall 2012**.
31. Connor MA, Menke AM, Vrcek I, Shore JW. Operating room fires in periocular surgery. *Int Ophthalmol* 2018; **38**: 1085-93.
32. Spigelman AD, Swan JR. Skin antiseptics and the risk of operating theatre fires. *ANZ J Surg* 2005; **75**: 556-8.
33. Tooher R, Maddern GJ, Simpson J. Surgical fires and alcohol-based skin preparations. *ANZ J Surg* 2004; **74**: 382-5.
34. Sunkara PR, Grauer JS, John J, Jones EL, Roy S, Cramer JD. Surgical Fires Involving Alcohol-Based Preparation Solution, 1991-2020. *Laryngoscope* 2023.
35. Jones EL, Overbey DM, Chapman BC, et al. Operating Room Fires and Surgical Skin Preparation. *J Am Coll Surg* 2017; **225**: 160-5.
36. AAGBI. Patient fire, 2018. [https://anaesthetists.org/Portals/0/PDFs/QRH/QRH\\_3-7\\_Patient\\_fire\\_v1.pdf?ver=2018-07-25-112714-097](https://anaesthetists.org/Portals/0/PDFs/QRH/QRH_3-7_Patient_fire_v1.pdf?ver=2018-07-25-112714-097) (accessed 11/7/2023).
37. Griffin B, Cabilan CJ, Ayoub B, et al. The effect of 20 minutes of cool running water first aid within three hours of thermal burn injury on patient outcomes: A systematic review and meta-analysis. *Australas Emerg Care* 2022; **25**: 367-76.
38. Mai CL, Wongsirimeteekul P, Petrusa E, et al. Prevention and Management of Operating Room Fire: An Interprofessional Operating Room Team Simulation Case. *MedEdPORTAL* 2020; **16**: 10871.
39. APSF. OR Fire Prevention Algorithm, 2014. <https://www.apsf.org/wp-content/uploads/collateral/posters/ORFireAlgorithmPoster22x28.pdf> (accessed 12/07/2023).